



Agenzia nazionale per le nuove tecnologie, l'energia
e lo sviluppo economico sostenibile



Ministero dello Sviluppo Economico

RICERCA DI SISTEMA ELETTRICO

Identificazione e collaudo di un sistema di misura non intrusivo per i
profili di velocità in piombo. Specifica tecnica di fornitura e
documentazione relativa all'installazione e collaudo

I. Di Piazza, G. Galgani, M. Tarantino

Report RdS/2012/051

IDENTIFICAZIONE E COLLAUDO DI UN SISTEMA DI MISURA NON INTRUSIVO PER I PROFILI DI VELOCITA' IN PIOMBO. SPECIFICA TECNICA DI FORNITURA E DOCUMENTAZIONE RELATIVA ALL'INSTALLAZIONE E COLLAUDO.

I. Di Piazza, G. Galgani, M. Tarantino - ENEA

Settembre 2012

Report Ricerca di Sistema Elettrico

Accordo di Programma Ministero dello Sviluppo Economico - ENEA

Area: Governo, gestione e sviluppo del sistema elettrico nazionale

Progetto: Nuovo nucleare da fissione: collaborazioni internazionali e sviluppo competenze in materia nucleare

Responsabile del Progetto: Mariano Tarantino, ENEA

Titolo

Identificazione e collaudo di un sistema di misura non intrusivo per i profili di velocità in piombo. Specifica tecnica di fornitura e documentazione relativa alla installazione e collaudo

Descrittori

Tipologia del documento: Specifica Tecnica di Fornitura
Collocazione contrattuale: Accordo di programma ENEA-MSE: tema di ricerca "Nuovo nucleare da fissione"
Argomenti trattati: Tecnologia dei metalli liquidi
 Termoidraulica dei reattori nucleari
 Generation IV Reactors

Sommario

Nel presente documento è riportata integralmente la specifica tecnica di fornitura di un misuratore di portata ad induzione elettromagnetica da installare sull'impianto a metallo liquido pesante NACIE. Sono inoltre allegati i seguenti documenti: la nota di consegna dello strumento, il Commissioning report sull'installazione e calibrazione in situ ed il manuale di istruzioni.


Note

Autori: I. Di Piazza, G. Galgani, M. Tarantino

Copia n.

In carico a:

2			NOME			
			FIRMA			
1			NOME			
			FIRMA			
0	EMISSIONE	18/09/2012	NOME	I. Di Piazza	A. Del Nevo	M. Tarantino
			FIRMA	<i>I. Di Piazza</i>	<i>A. Del Nevo</i>	<i>M. Tarantino</i>
REV.	DESCRIZIONE	DATA	HEDAZIONE	CONVALIDA	APPROVAZIONE	

	Sigla di identificazione NNFISS – LP3 - 042	Rev. 0	Distrib. P	Pag. 2	di 8
---	---	------------------	----------------------	------------------	----------------

Index

OVERVIEW..... 3

SCOPE OF THE SUPPLY 4

DOCUMENTATION FOLLOW UP 5

CALIBRATION SET-UP BY ENEA..... 5

DELIVERY TIME 6

PAYMENTS..... 6

GUARANTEE, PENALTIES, SHIPMENT..... 6

ANNEX I: FLOW METER TECHNICAL SPECIFICATION 7

REFERENCES..... 8

OVERVIEW

In the frame of the research activities planned to support the development of a Lead cooled Fast Reactor (LFR), ENEA assumed the commitment to run experimental tests to simulate the thermal-hydraulic behavior of a pin fuel bundle cooled by heavy liquid metal.

These activities, which will be performed in the context of the Program Agreement between ENEA and Ministry of Economical and Sustainable Development (MSE), will be carried out on NACIE (NAtural Circulation Experiment) facility loop, located by ENEA Brasimone Research Centre.

NACIE ([1], [2]) is a rectangular loop facility which allows to perform experimental campaigns in the field of the thermal-hydraulics, fluid-dynamics, chemistry control and heat transfer and to obtain correlations essential for the design of nuclear systems cooled by heavy liquid metals. A sketch of NACIE is shown in Fig. 1. It basically consists of two vertical pipes (O.D. 2.5”), working as riser and downcomer, connected by two horizontal pipes (O.D. 2.5”). In the bottom of the riser a heat source is installed, while a heat exchanger is placed in the upper part of the downcomer.

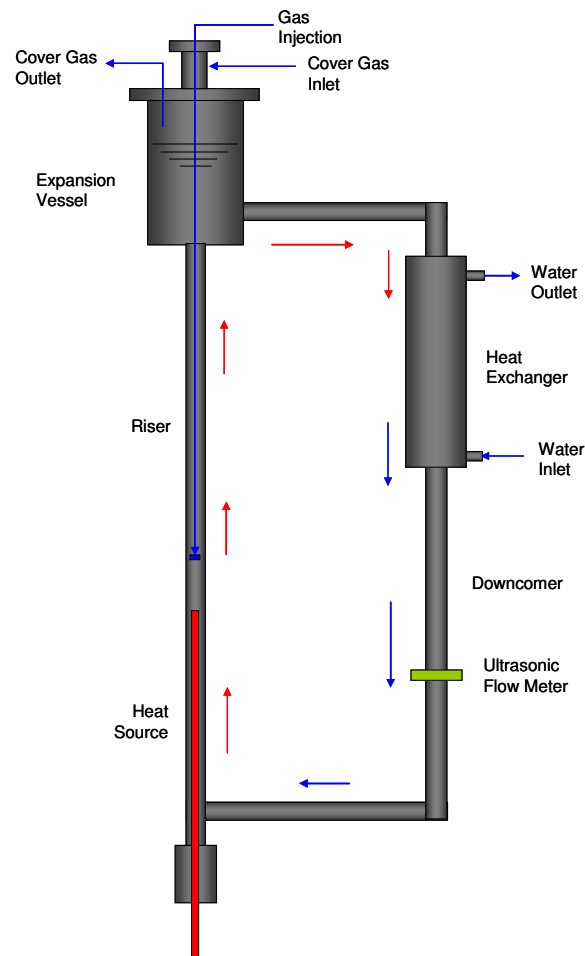



Fig. 1: Sketch of the NACIE facility.

NACIE is made in stainless steel (AISI 304) and can use both lead and the eutectic alloy LBE as

	Sigla di identificazione	Rev.	Distrib.	Pag.	di
	NNFISS – LP3 - 042	0	P	4	8

working fluid (about 1000kg). The loop has been designed to work up to 10 bar and 550°C. NACIE allows both natural and enhanced circulation regime. Enhanced circulation measurements are realized injecting Argon gas at the bottom of the riser, immediately above the heat source. The gas promotes the circulation of the LBE and is recaptured in the expansion vessel above the riser.

The heat source will consist of 19 electrical pins with a heat flux of $q'' = 1 \text{ MW/m}^2$. The bundle will be closed by a hexagonal wrapper. The total power of the new pin fuel bundle is $\approx 235 \text{ kW}$.

An inductive flow meter will be installed on NACIE to allow accurate measurements, to be supplied by HZDR, which has a wide experience with the measuring techniques with Liquid Metals.

In the past the HLM flow rate has been estimated applying a heat balance through the heat source [3]; the proposal is to apply this methodology to calibrate on site the inductive flow meter which will be supplied.

The goals of the experimental campaigns planned on the NACIE loop facility with the new inductive flow meter and the new heat source are:

- the measurement of the pin wall temperature;
- the measurement of the subchannel temperature;
- the characterization of hot spots points;
- the observation of the axial thermal stratification of the coolant fluid and its entrance length in the bundle subchannels;
- the measurement of the mass flow rate of LBE during natural and gas enhanced circulation experiments.

The new flow meter will be an inductive phase-shift sensor able to measure the perturbation of the magnetic field by the flow. It is characterized by a high temporal resolution and it can be applied at high temperature (up to 450°C).

A sketch of the new flow meter for NACIE is shown in Fig. 2 (image from HZDR)

SCOPE OF THE SUPPLY

The aim of the Supply is

- the procurement of an inductive flow meter able to measure mass flow rate with HLM, in a range of temperature of 150 – 450 °C and in a range of velocity of 0.1 – 2 m/s;
- the procurement of the electronic equipment needed to properly operate the sensors;
- the shipment of the components by the C.R. ENEA Brasimone, Italy;
- support for the installation of the sensor on NACIE loop; for this purpose, the thermal insulator (100 mm thickness) and the heating cable (O.D. 10 mm) will be removed from the

pipe zone where the sensor will be installed, for a maximum length of 200 mm.

- support for the on-site calibration of the flow meter on the NACIE loop;
- support on-site for a past-evaluation of the sensors performance (if required by ENEA)

The flow rate will be installed on NACIE loop, in the vertical pipe downstream the heat exchanger.

The flow rate sensor will remain at ENEA after the installation.

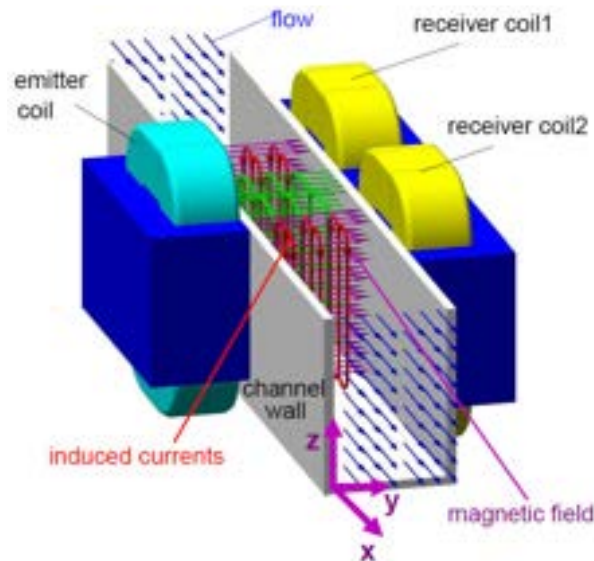


Fig. 2:Sketch of the new inductive flow meter for NACIE.


DOCUMENTATION FOLLOW UP

The supply will be completed by a documentation set follow up. The following documents will be delivered:

- Inductive Flow Meter: Scientific Background, Installation and Operation Handbook
- Pre-calibration Report
- Calibration procedure on site
- End of Manufacturing, Performed tests and Calibration Report

All the documents will have to be reviewed by ENEA (usually one week is allocated for that action).

CALIBRATION SET-UP BY ENEA

 ENEA Ricerca Sistema Elettrico	Sigla di identificazione	Rev.	Distrib.	Pag.	di
	NNFISS – LP3 - 042	0	P	6	8

The calibration set-up of the flow meter will be performed by ENEA on the NACIE loop, by the HZDR support on site.

The Supplier will communicate two weeks before the calibration on-site the actions to be performed on the loop aiming to properly install the flow meter (i.e. length of the free part for the sensors installation).

DELIVERY TIME

The flow meter has to be delivered within three months after the order.

The on-site calibration will take place within two months after the delivery of the flow meter.

PAYMENTS

- 30% of the total selling price after the delivery of the following documentation:
 - Inductive Flow Meter: Scientific Background, Installation and Operation Handbook.
 - Pre-Calibration Report.
- 40% of the total selling price after the delivery of the sensor and the related electronic equipment.
- 30% of the total selling price after the calibration on site and the delivery of the documents
 - Calibration procedure on site.
 - End of Manufacturing, Supply and Calibration Report.

The Payments will be performed by Bank Transfer within 30 days after the invoice.

GUARANTEE, PENALTIES, SHIPMENT

The supplier will not be responsible concerning the performance of the flow meter.


Anyway the sensors and the electronic equipment will be guaranteed for a period of 24 months after the delivery.

In case of a delay on the delivery, a liquidity damage of 0.3% of the total selling price a week with a maximum limited to 10% of the total selling price will be applied.

The shipment will be Delivered Duty Unpaid (DDU), by the C.R. ENEA Brasimone, Italy, packaging free of charge.

ANNEX I: FLOW METER TECHNICAL SPECIFICATION

<u>NACIE (LBE loop)</u>	
Outer Diameter Pipe	73.02 mm
Inner Diameter Pipe	62.7 mm
Thickness Pipe	5.16 mm
Temperature	150 – 450 °C
Velocity	0.1 – 2 m/s
Mass flow rate	3 – 65 kg/s
Density range	10,140 – 10,535 kg/m ³
Latent heat of melting at the normal melting point	38.5 kJ/kg
Boiling point	1,670 °C
Heat of vaporisation at the normal boiling point	854 kJ/kg
Saturation vapour pressure	$7.93 \times 10^{-14} - 3.17 \times 10^{-4}$ Pa
Surface tension	0.389 – 0.409 N/m
Thermal expansion	$1.26 \times 10^{-4} - 1.31 \times 10^{-4}$ K ⁻¹
Sound velocity	1,699 – 1,766 m/s
Heat capacity at constant pressure	143 – 149 J/kg K
Dynamic viscosity	$1.40 \times 10^{-3} - 2.94 \times 10^{-3}$ Pa s
Kinematic viscosity	$1.4 \times 10^{-7} - 2.8 \times 10^{-7}$ m ² /s
Electrical resistivity	$1.08 \times 10^{-6} - 1.23 \times 10^{-6}$ Ω m
Thermal conductivity	10.3 – 14.6 W/m K
Working Time (per year)	3000 h

	Sigla di identificazione NNFISS – LP3 - 042	Rev. 0	Distrib. P	Pag. 8	di 8
---	---	------------------	----------------------	------------------	----------------

REFERENCES

- [1] “*Natural circulation in a liquid metal one dimensional loop*”, M. Tarantino, S. De Grandis, G. Benamati, F. Oriolo, *Journal of Nuclear Materials*, 376 (2008), 409 - 414.
- [2] “*Experimental Investigation of the Thermal – Hydraulic behaviour of Heavy Liquid Metal Cooled Reactors*”, M. Tarantino, Ph.D thesis, University of Pisa, Academic Years 2005 – 2007.
- [3] “*Natural and gas enhanced circulation tests in the NACIE Heavy Liquid Metal loop*”, M. Tarantino, D. Bernardi, G. Coccoluto, P. Gaggini, V. Labanti, Proceedings of ICONE 18, 18th International Conference in Nuclear Engineering, May 17 – 21, Xi’an, China.



Helmholtz-Zentrum Dresden Rossendorf
Bautzner Landstraße 400
01328 Dresden, Germany

To:
ENEA
Experimental Engineering Technical Unit
Brasimone Research Center
40032 Camugnano Bologna
Italy

Delivery order

For a contactless, electromagnetic flow meter,

referring to order:

CJG No. 318 206 4248,
CUP No. J31 J11 000 13 000 6

1) Manual instruction (cfr sensor)

Herewith we confirm the receipt of a manual instruction for a contactless electromagnetic flow meter including all necessary specifications and technical details. Furthermore all details of mechanical and electrical adjustments are contained with a guidance of calibration.


Signature (ENEA):

A handwritten signature in black ink, reading "Ivan Di Pace". The signature is written in a cursive, flowing style with a long horizontal line extending to the right.

2) *Contactless, electromagnetic flow meter (cfr sensor)*


Included Components

The delivered flow meter device consists of the measuring element and a supply/analysis unit.

Signature (ENEA): 

Installation at the NACIE-loop, ENEA-Brasimone

Measuring element as well as the supply- and analysis unit will be installed at the NACIE loop. An electro-mechanical adjustment of the device for stable operation is included.

Signature (ENEA): 

Calibration of the device at NACIE-loop, ENEA-Brasimone

The flow meter has to be calibrated for specified flow rates and operational temperatures (calibration letter).

Signature (ENEA): 



Helmholtz-Zentrum Dresden Rossendorf
Bautzner Landstraße 400
01328 Dresden, Germany

To:
ENEA
Experimental Engineering Technical Unit
Brasimone Research Center
40032 Camugnano Bologna
Italy

| Commissioning report

referring to order:

CJG No. 318 206 4248,
CUP No. J31 J11 000 13 000 6

| Editor: Dr. D. Buchenau (HZDR)

Dresden, den 12.07.2012

Helmholtz-Zentrum Dresden-Rossendorf e.V. ; Bautzner Landstraße 400, 01328 Dresden;
Vorstand: Prof. Dr. Roland Sauerbrey, Prof. Dr. Dr. h. c. Peter Joehnk; VR 1693 beim
Amtsgericht Dresden

The following commissioning report relates to the works performed in the period from Tuesday (02.07.2012) to Wednesday (03.07.2012). All steps with respect to the preparation and execution of the commissioning phase of the inductive flow meter at the NACIE loop were carried out by the following nominated persons as members of the Helmholtz-Zentrum Dresden-Rossendorf (HZDR) and the SAAS-GmbH.

Dr. D. Buchenau

HZDR, Institute of Fluidynamics, Department of Magnetohydrodynamics, 01328 Dresden, Bautzner Landstraße 400, Germany.

Dr. S. Lenk

SAAS-GmbH, 01728 Bannewitz/Possendorf, Poisentalsstraße 03, Germany

M. Flöter

SAAS-GmbH, 01728 Bannewitz/Possendorf, Poisentalsstraße 03, Germany

The customer is represented by the following person:

Dr. Ivan Di Piazza

ENEA, UTIS-TCI C.R. Brasimone, 40032 Camugnano (Bo), Italy.

Following steps during installation and calibration of the contactless flow meter EMD-ps were performed:

Period	Results
3.7.2012 9:00 to 13:00 o'clock	Assembly of the sensor system including mechanical adjustment of the system and installation of all necessary electrical connections between supply/measurement unit and sensor head at the NACIE-facility.
3.7.2012 14: 00 to 17:00 o'clock	Basic functional tests. Adjustment of all necessary parameters of the sensor system, Admission of ENEA costumers to the device based on the delivered manual instruction.
3.7. 2012 17:00 to 4.7.2012 9:00 o'clock	Heating of the NACIE-loop to an operational temperature of 300°C. Periodically appearing fluctuations of the sensor output at a fixed

Helmholtz-Zentrum Dresden-Rossendorf e.V. ; Bautzner Landstraße 400, 01328 Dresden; Vorstand: Prof. Dr. Roland Sauerbrey, Prof. Dr. Dr. h. c. Peter Joehnk; VR 1693 beim Amtsgericht Dresden

	loop temperature were observed. Presumably the fluctuations are caused by switching on and switching off heating elements of the loop causing an additional flow driven heat convection in the closed loop measured by the flow meter.
4.7.2012 9:00 to 13:00 o'clock	Calibration of the contactless flow meter with a buoyant driven flow at a fixed temperature. The flow rate of liquid metal in the loop is adjustable by an Argon injector. The Argon flow rate was determined in NL/min (Tab. 1). The adjusted/generated flow rate was determined by a temperature equilibrium measurement located close to a heating element (10-20 kW). According to ENEA the used calibration process delivers flow rates within a measurement uncertainty of approx. 10% (Tab. 1).

<i>Volume flow rate (Argon)</i>	<i>Calculated mass flow rate</i>
0 NL/min	0 kg/s
1 NL/min	10,1 kg/s
2 NL/min	12,4 kg/s
6 NL/min	16,5 Kg/s

Tab. 1: Adjusted Argon flow rates and calculated mass flow rates.

<i>Volume flow rate</i>	<i>Calculated mass flow rate</i>	<i>Result / Sensor</i>
0 NL/min	0 kg/s	0,02 kg/s
1 NL/min	10,1 kg/s	11,3 kg/s
2 NL/min	12,4 kg/s	12,4 -12,6 kg/s
6 NL/min	16,5 Kg/s	18,4 kg/s

Tab. 2: Calibration points of the contactless flow meter.

4.7.2012 14:00 to 16:00 o'clock	Measurements in the Tab. 2 were taken at a loop temperature at 300°C. Different calibration points were adjusted and compared with the flow meter measurements. Reproducibility and zero drift were compared within the agreed conditions of contract.
---------------------------------	--

EMD *ps*

Manual / Operating Instruction

Content:

1. Functionality and Application of the Device	3
2. Information for the Electrical Safety	6
3. Installation and Wiring	7
4. Initiation and Symmetry Alignment.....	11
5. Menu for the Operating of the Device	13
5.1. "Measurement" – Measurement Value, Error Notifications	13
5.2. "System Setup" – Input of System Parameters (secured by password).....	14
5.3. „ Channel Setup" – Input of Channel Parameters (secured by password)	15
5.4. „Calibration" – Two Point Calibration, Zero Point Calibration	16
5.5. „Service" – Measurement value control	17
6. Analog Output of EMD μ s	18
7. USB-Interface for Data Storage	19
8. Technical data sheet	20

1. Functionality and Application of the Device

The device EMD ρ_s is intended for the recording of the flow rate for liquid metal in pipes. The measurement principle is based on the recording of current dependent distortions of phases induced by alternating voltage. The alternating voltage is induced into the fluid by a transmitter coil. A receiving coil which is also placed in the flow channel detects the induced voltage. A distortion in phases exists between the sent and received voltage, which is linear related to the average flow velocity of the fluid (Fig. 1).

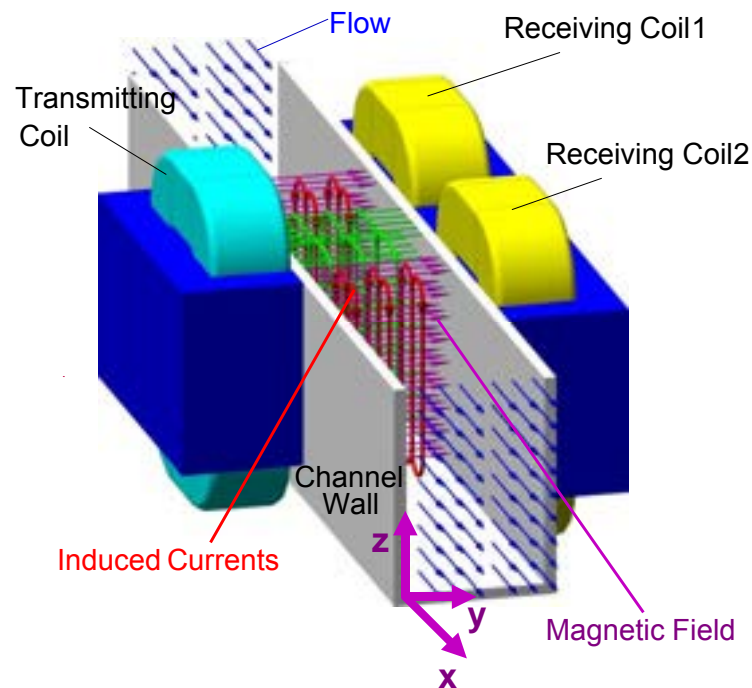


Fig.1 Principle of Measurement (origin from HZDR)

The measuring device consists of the following:

- Sensor unit, to be assembled on a pipe
- Evaluating unit transducer wall mounted

The maximum distance (cable length) between the sensor and transducer is 20m.

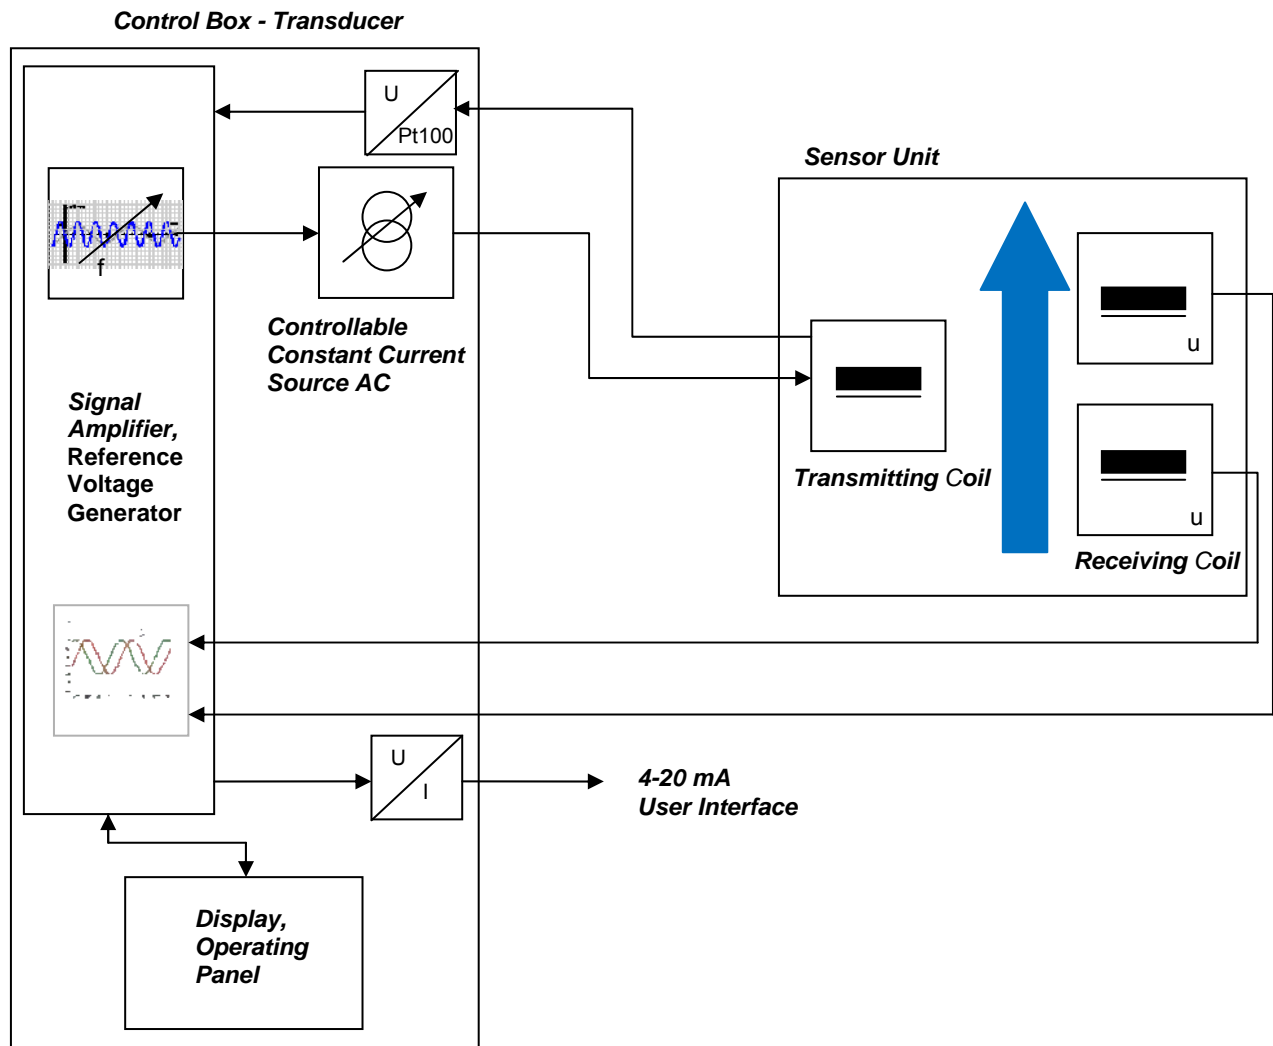


Fig. 2: Block Diagram of **EMD ps**

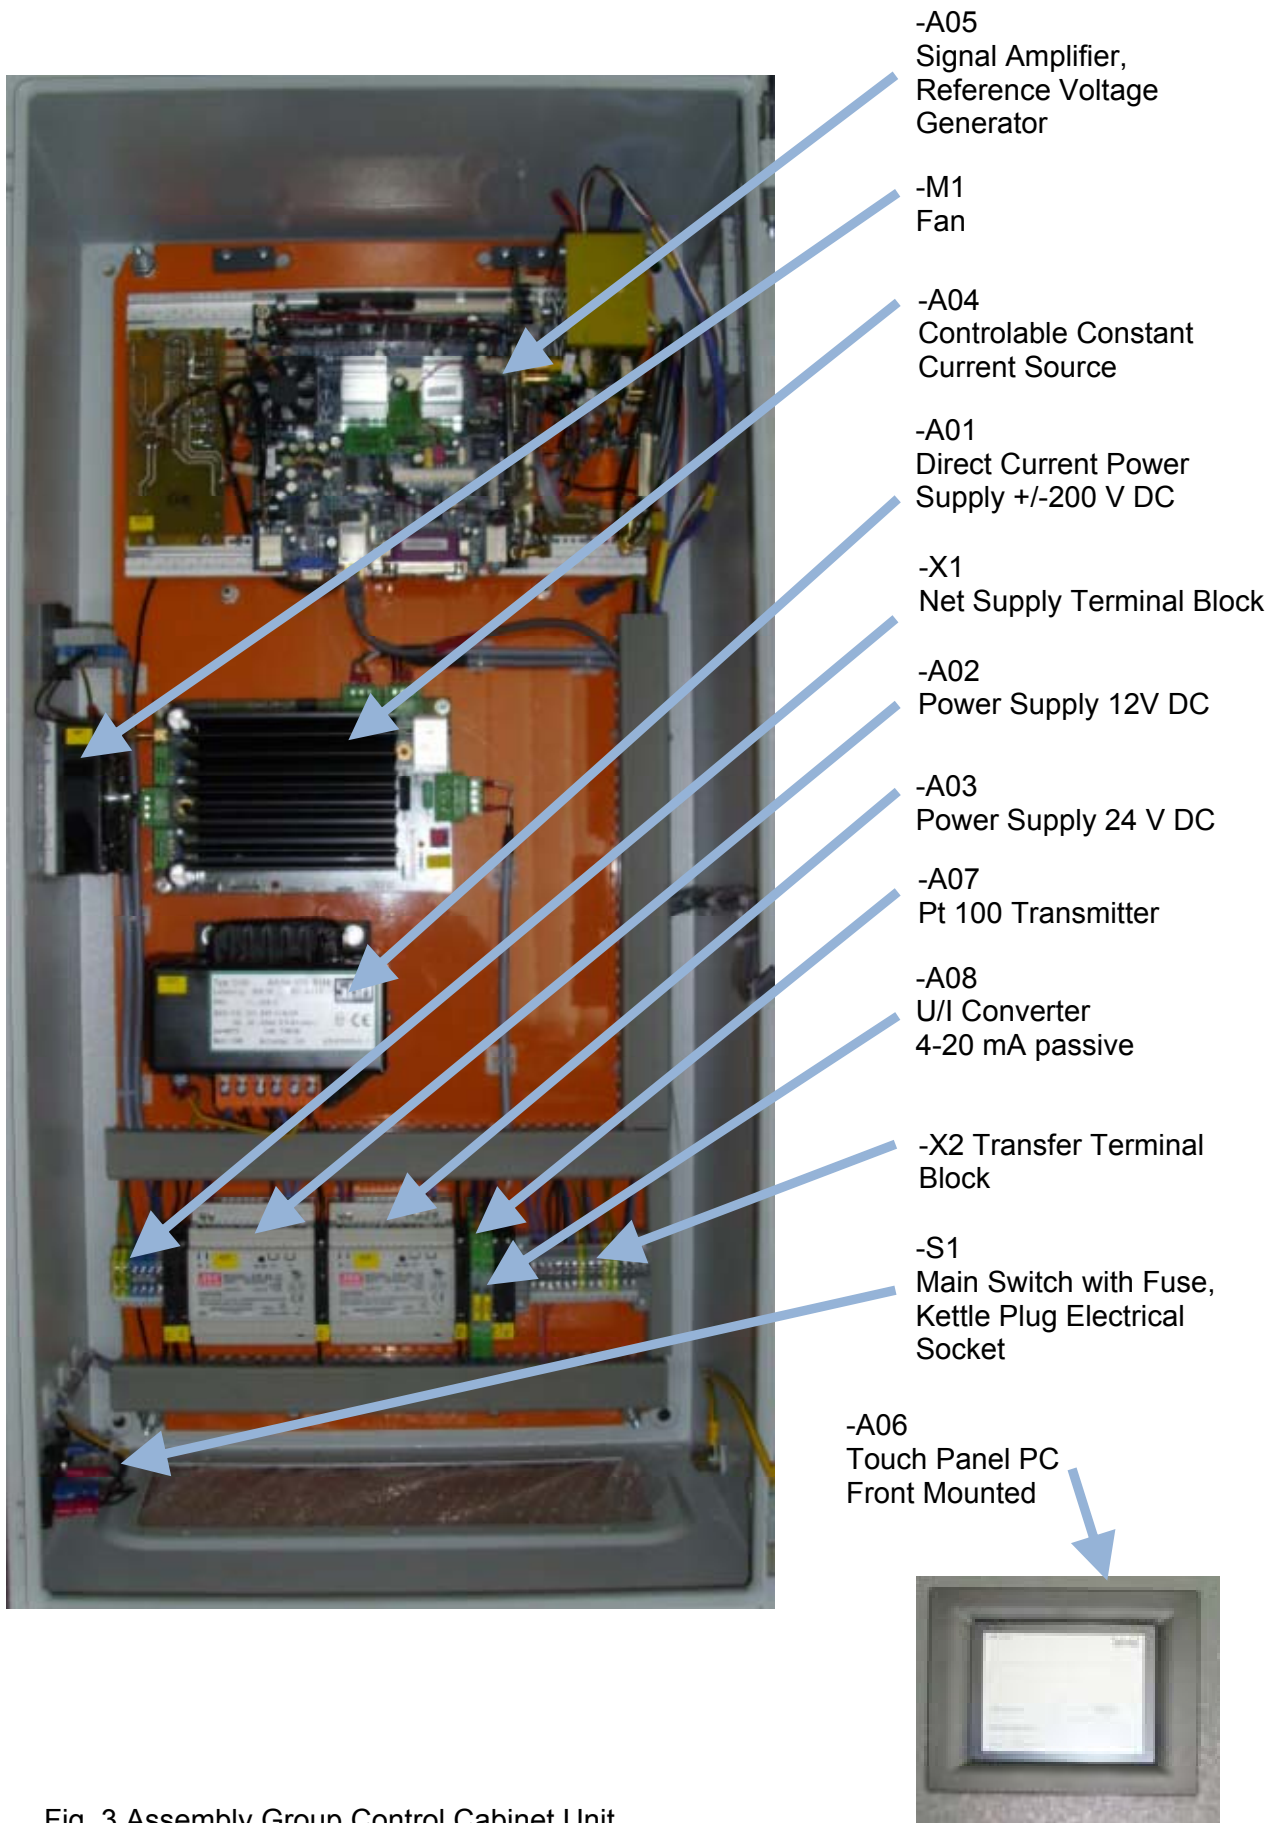


Fig. 3 Assembly Group Control Cabinet Unit

2. Information for the Electrical Safety


The control cabinet unit is operating with a power supply with kettle plug.

**Before Opening the Device Remove the Power Plug!
Energized Parts up to 200 V DC!**



The power supply voltage of transmitting coil is +/- 200 V DC

**Before Opening the Sensor Casing Disconnect
Induction Current Supply
(Open Fuse Clip -F5, -F6)!**

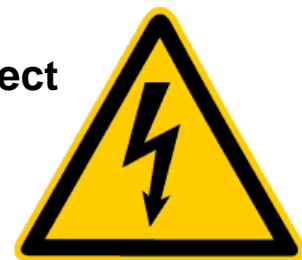

**Do Not Disconnect 200 V DC
Power Supply from Signal Amplifier!
Danger Because of Residual Voltage at the
200 V DC Power Supply Module after
Supply Voltage 230 V AC Was Switched off!**



The device has the degree of protection IP 54 and is therefore suitable for usage in dry and frost-free rooms.



**Inside of the Control Box Is Not
Completely Screen Protected against
Electric Shocks!**




3. Installation and Wiring

Step 1: Installation of Control Box - Transducer

The control box is designed for wall installation

Dimensions:

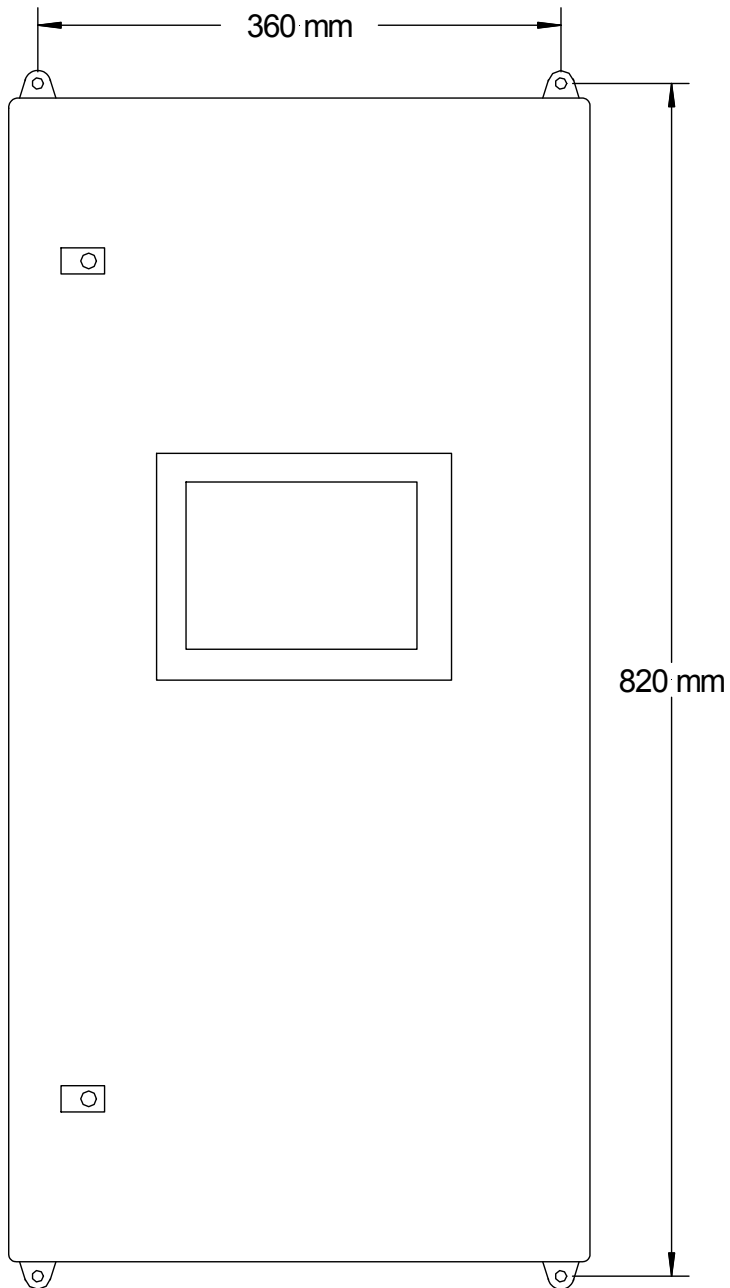

Detail:

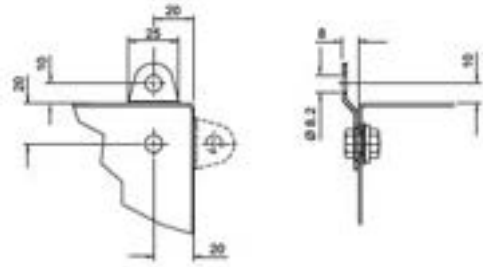


Fig. 4 Wall Fastening of Control Box -Transducer

Step 2: Sensor Installation on the Pipe:

The sensor unit consists of two symmetrical components, after removing the sensor casing (1), which are mounted around the pipe with the stream to be captured and (2) the aluminum clamps (1) which were constructed custom-fit to stream pipe, that secure the sensor. The measured positive direction of fluids flow is marked with an arrow.

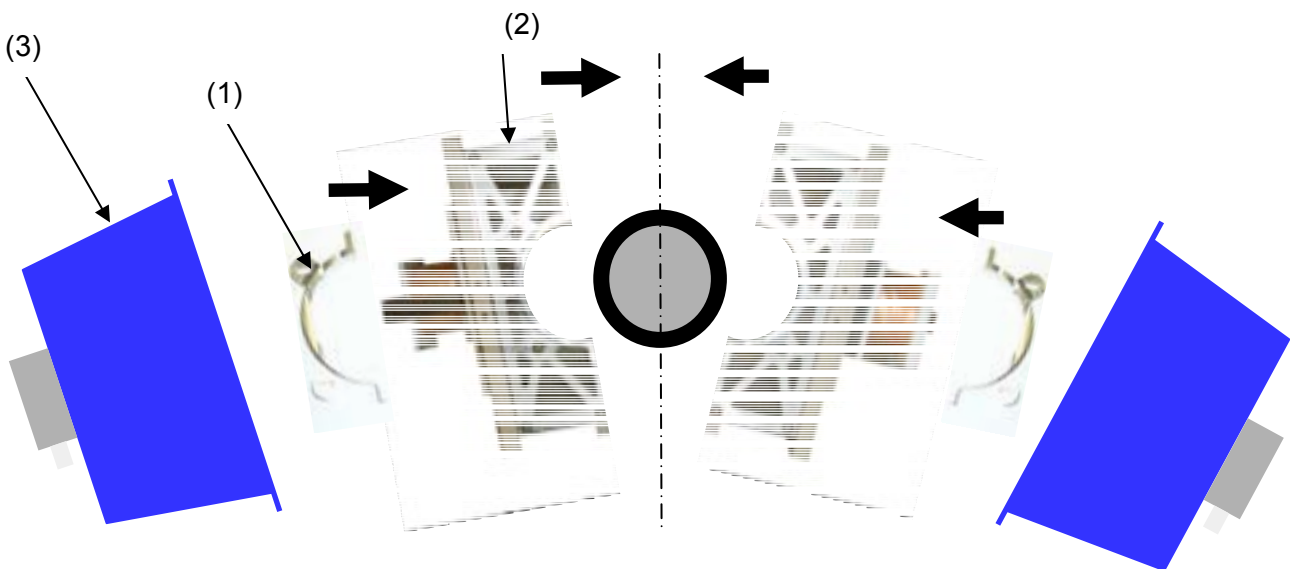
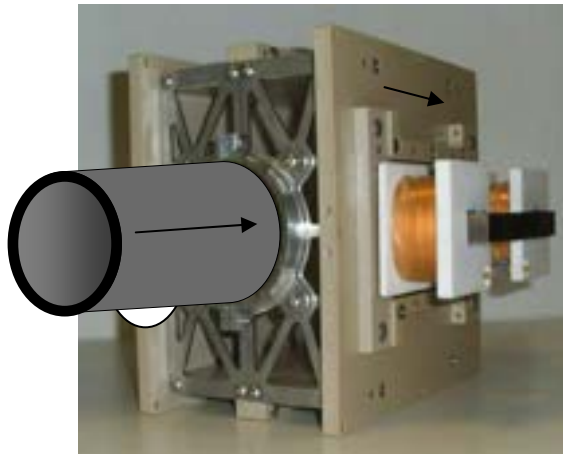


Abb. 5 Sensor Unit Assembling

Step 3: Attachment of the Sensor Unit and the Control Cabinet without the Sensor Casing.

For this purpose, the wires W100, W101, W102 and W103 are used to extend the connection between the coils and the control box -transducer. The sensor casing (3) Fig. 5 should be kept clear as far away as possible during the adjustment of the sensor, to minimize the influence of the alternating field. The wiring between the sensor and the control cabinet is to be carried out suitable to local terms. The wire W101 has to have a distance of 100mm minimum to the wires W102 and W103.

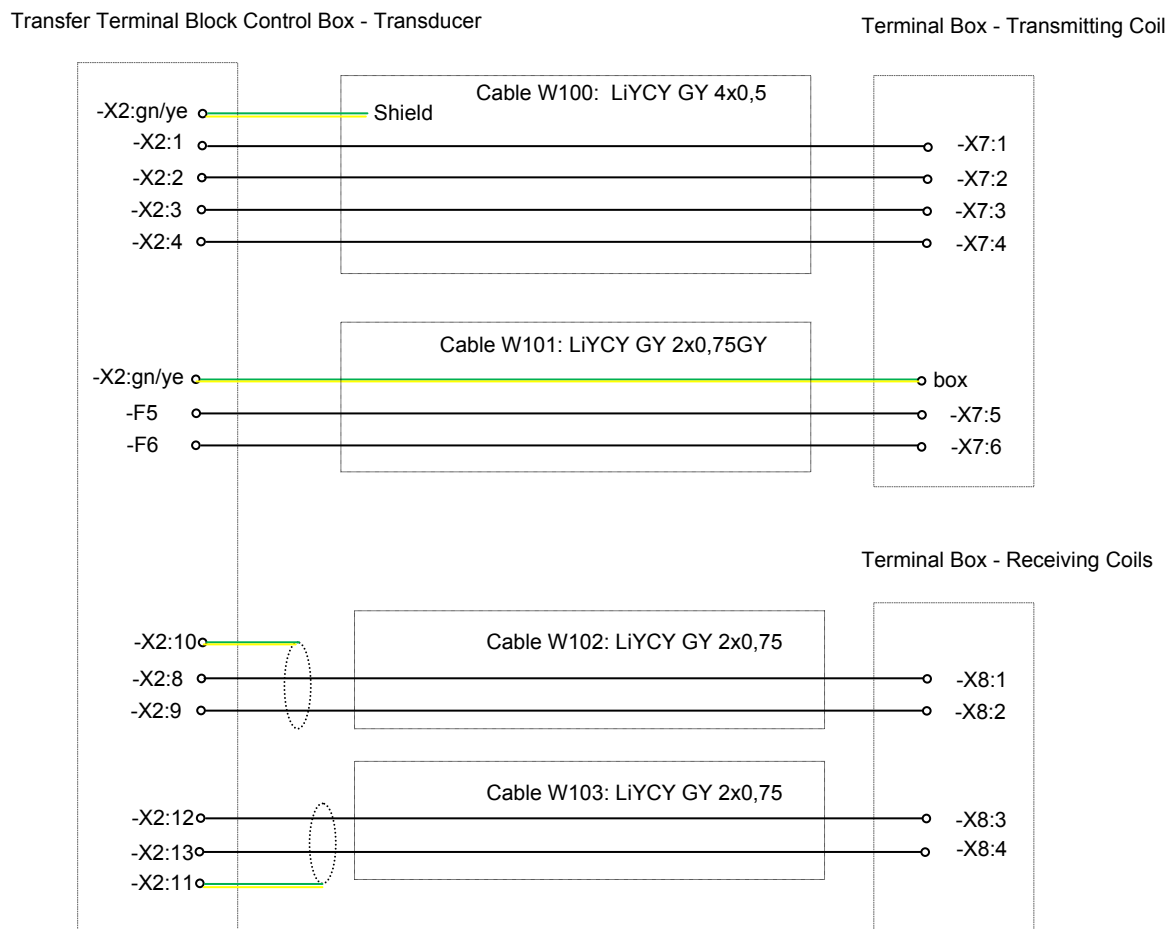


Fig. 6: General Wiring Diagram Sensor Unit – Control Box - Transducer

For equipotential bonding the following connections (Fig 7) have to be realised:

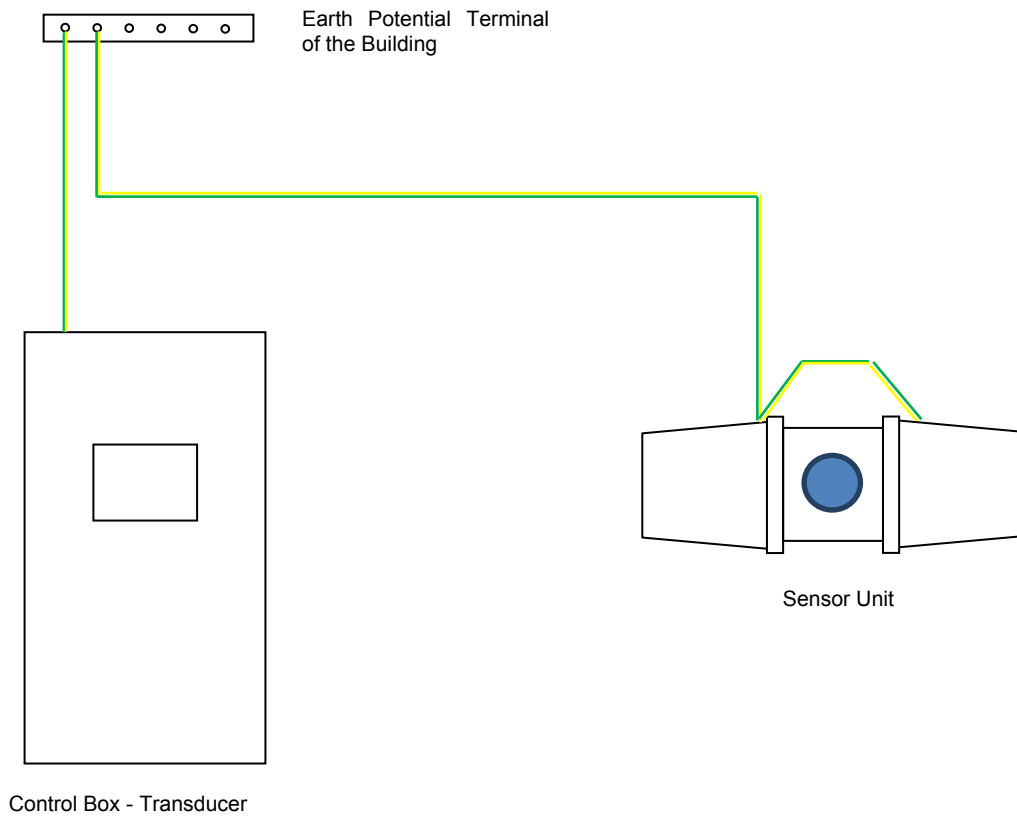


Fig.: 7 Equipotential Bonding between the EMD Components


4. Initiation and Symmetry Alignment

Completely wired and assembled, the device can also be launched by turning on the main switch, even if the device has a sensor without a sensor casing.

The error code is 0000H and green, if all components are working correctly.

The Device Requires an Adaption Phase of about an Hour after Being Switched on.

The main operating parameters can be observed in the menu under Service. The excitation frequency and current and are bound to type and preset.

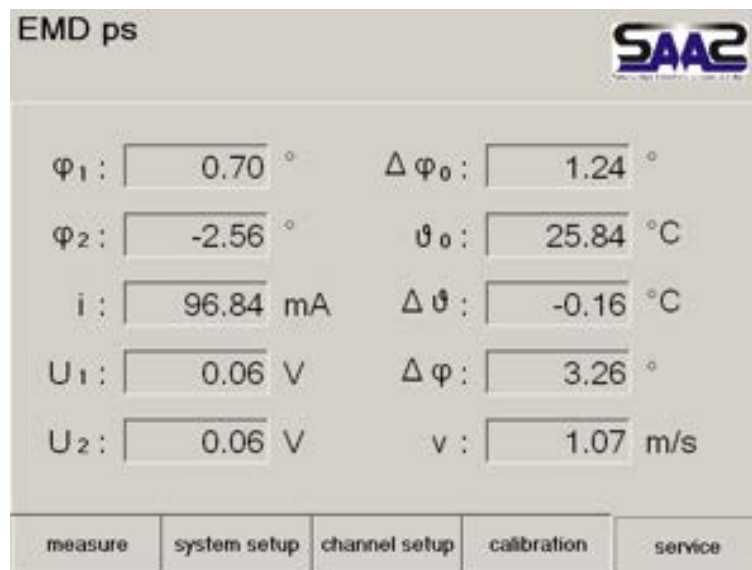

Objective of the implementing and adjustment is the preferably symmetrical distribution of the receiving magnetic field onto the receiving coils without flowing medium.

The main operating parameters can be observed in the menu under Service. The excitation frequency and current and are bound to type and preset.

Objective of the implementing and adjustment is the preferably symmetrical distribution of the receiving magnetic field onto the receiving coils without flowing medium.

The voltages u_1 and u_2 are to be adjusted as well as the minimization of the phase difference $\Delta\varphi$. This process is possible on both the sending and receiving side and if needed can be done on both these sides.

The procedure for this process is the following:

1. Remove lock pins (1), drive through with suitable tool, loosening the attachment bolts until one can move the core mounting (3)
2. Slide the core using the adjustment screws (4) until the induced voltage is the same and the phase difference is at its minimum.

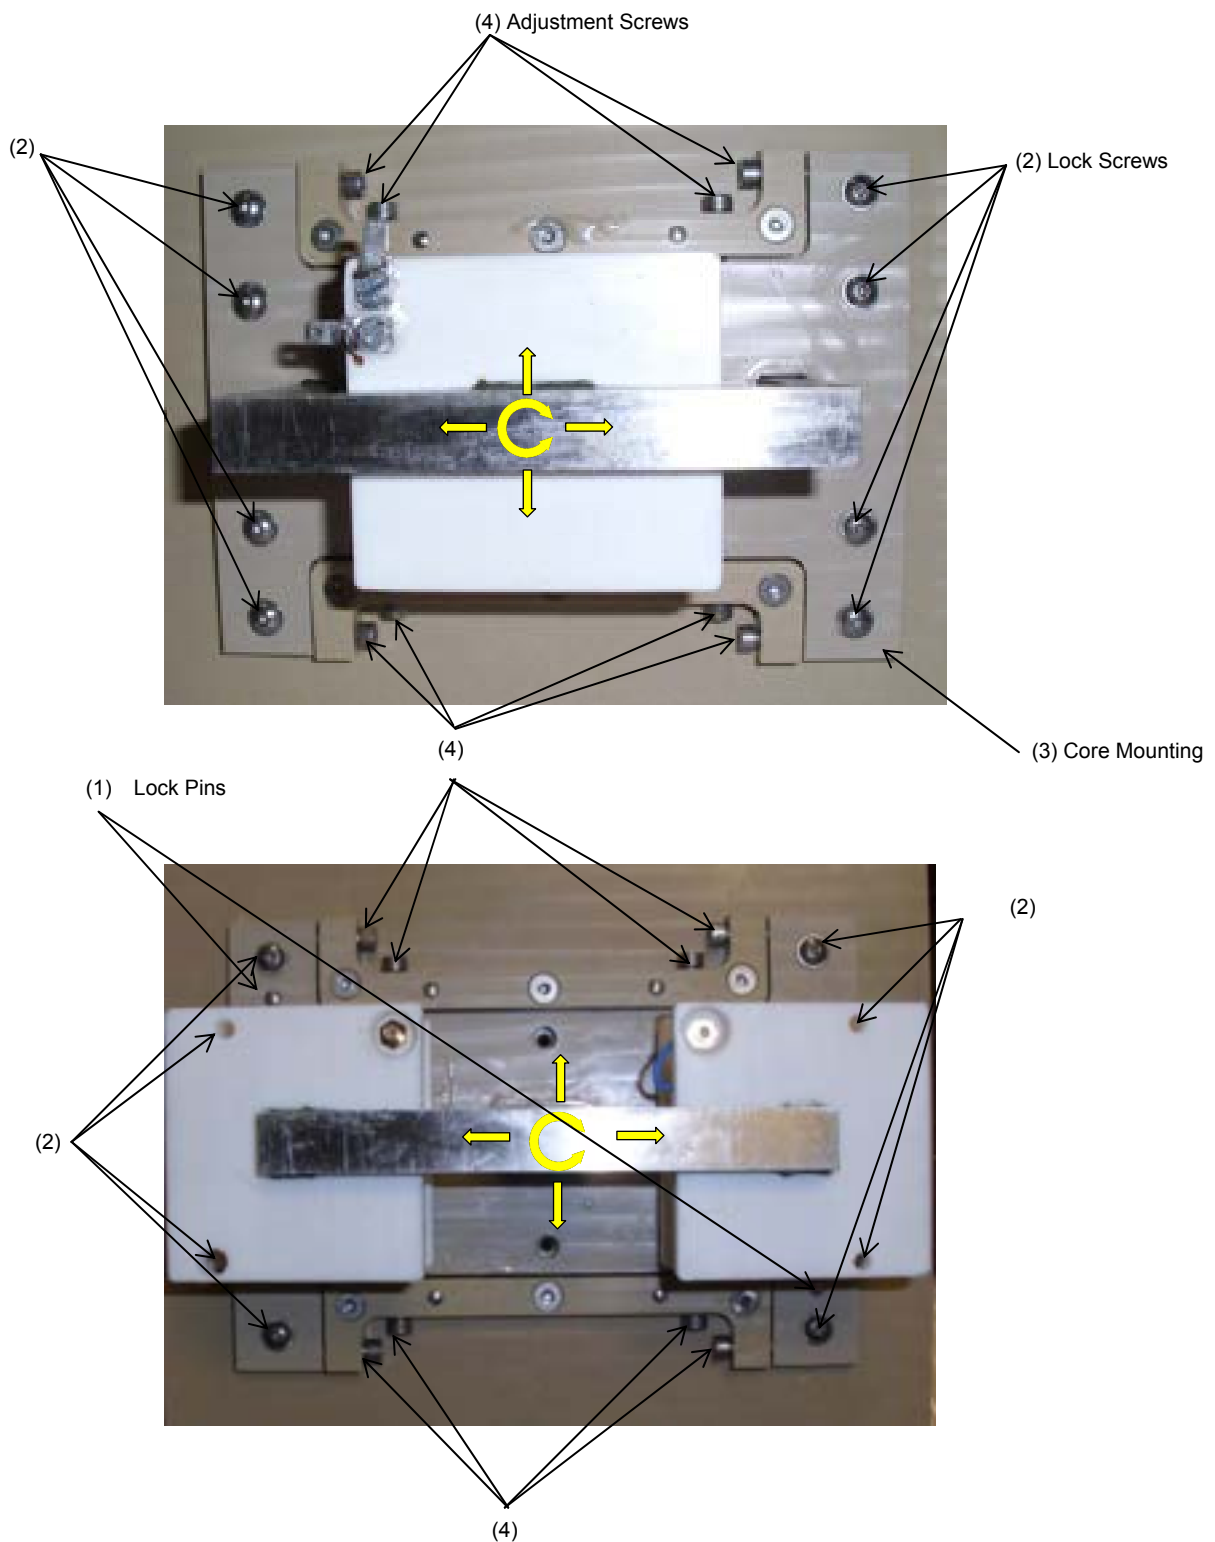



Fig. 8 Alignment of Sensor Unit

The result has to be checked after the installation of the sensor casing and may be readjusted.

5. Menu for the Operating of the Device

The device EMD *ps* used a touch panel to operate.

5.1. “Measurement” – Measurement Value, Error Notifications

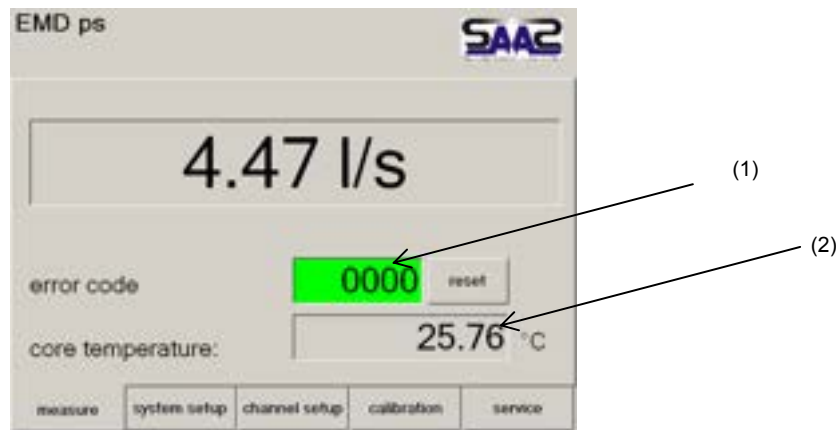


The error notification (1) is coded in hexadecimal notation. The error code is 0000 and green, if all components are working correctly. Warnings are marked yellow. Error notifications which lead to the shutdown of the excitation current or a downtime of the measurement are red. The error can be reset after removing the error source by using the reset button. The temperature of the magnetic core (2) gives information about the thermal situation around the sensor.

List of error notifications:

Position	Error	Description	Action
2 ⁰	SetErrormA	Measurement value out of range	Warning
2 ¹	CurrentFailure	Induction current out of range (deviation more than 10 % from set point)	ShutDown
2 ²	NoConnection	No connection between panel and signal amplifier	HoldOn
2 ³	Temperature Failure	Temperature measurement out of range, wire break	Warning
2 ⁴	U1Failure	Low voltage from transceiver coil 1	Warning
2 ⁵	U2Failure	Low voltage from transceiver coil 1	Warning
2 ⁶	CalibrationFailure	Result “ not a number” division by zero	Last calibration will be used further on
2 ⁷ - 2 ¹⁵	Unused		

5.2. "System Setup" – Input of System Parameters (secured by password)

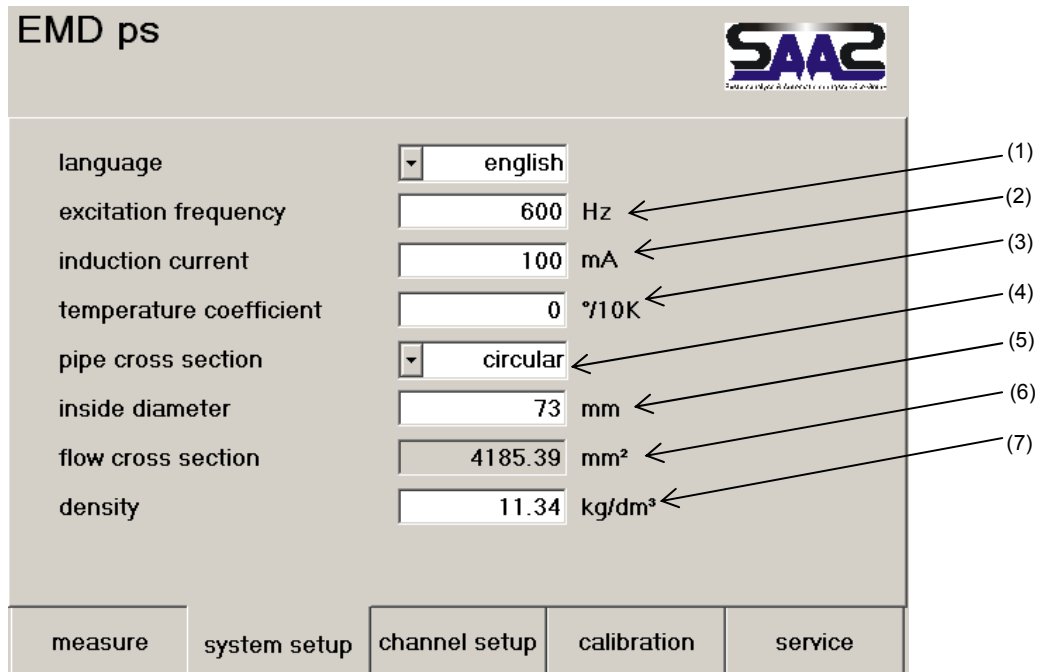

Parameter	Value	Unit	Label
language	english		(1)
excitation frequency	600	Hz	(2)
induction current	100	mA	(3)
temperature coefficient	0	%/10K	(4)
pipe cross section	circular		(5)
inside diameter	73	mm	(6)
flow cross section	4185.39	mm ²	(7)
density	11.34	kg/dm ³	

measure system setup channel setup calibration service

The input of the nominal value of excitation current is restricted to a maximum of 500mA (2).

The restriction for the excitation frequency is 300Hz (1).


The temperature coefficient of the measurement value (3) is dependent on the fluid and therefore has to be determined by it.

The preset values are sensor specific and should not be changed.

There is the possibility to either save the diameter (5) of the pipe by selecting circular (4) or the area (6) directly.

For the calculation of the flow stream the density (7) of the fluid can be set as a constant.

5.3. „ Channel Setup” – Input of Channel Parameters (secured by password)

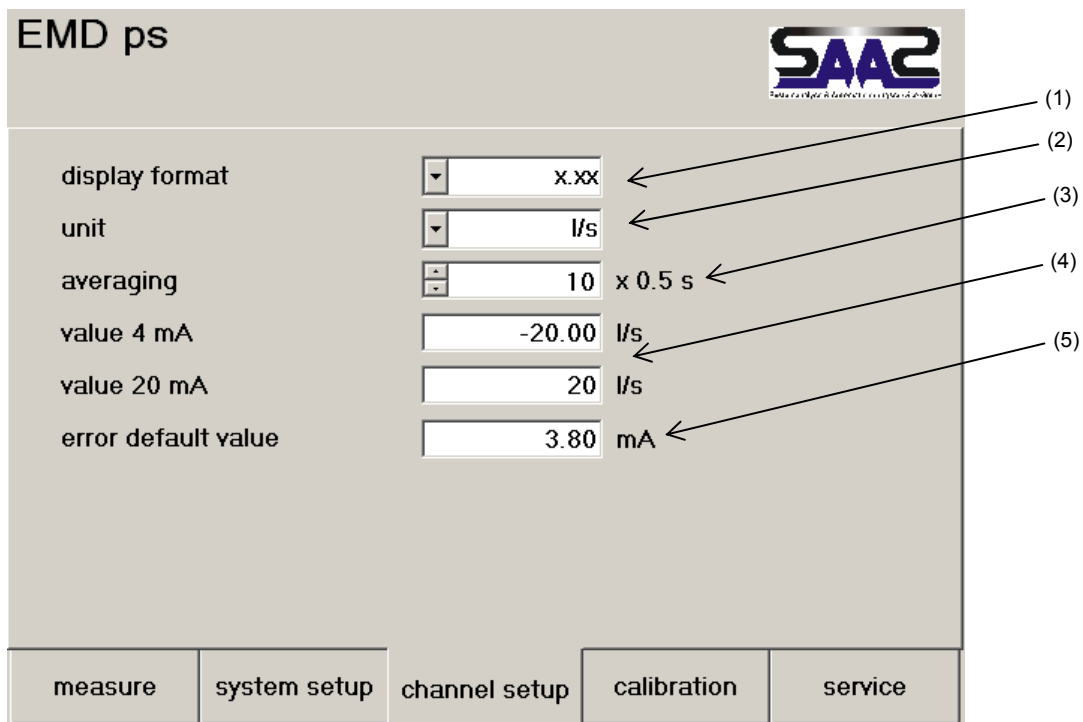

It is possible to determine 3 formats for the decimal place depending on the calibration of the display of the measurement value (1):

xxx xx,x x,xx

The following engineering units are available for the display of the measurement value (2):


l/s, l/min, m³/h, kg/s, t/h

The display value of the flow stream can be set to a moving average. A value is collected every 500ms. The input of 1 to 10 changes the duration of this cycle in multiples of 500ms (3). The device EMD ps has an analog output interface. Output is the displayed analog value. The dimensioning of the current output results from the ending points of the current range (4):

4 mA und 20 mA

In case of error, if no correct measurement value can be recorded, a preset value is being displayed (5).

5.4. „Calibration“ – Two Point Calibration, Zero Point Calibration

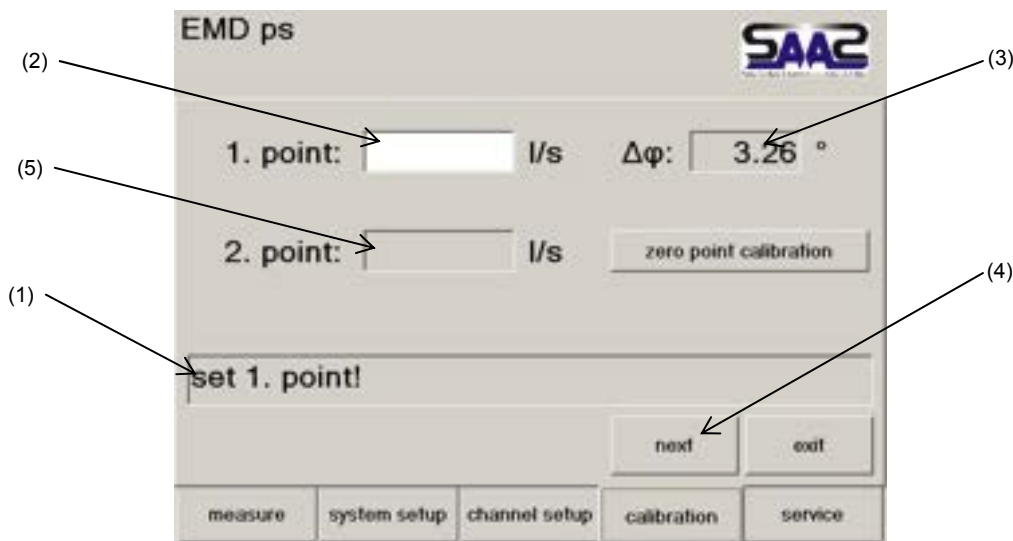

The device EMD ps has a linear characteristic line and is calibrated over two points. Since the device can determine the flow rate in both directions, the entry will not be verified for plausibility. Division by ZERO, due to an incorrect entry of calibration data will lead to a warning and interruption of the calibration.

See section 5.1 List of error notifications

Therefore the calibration consists of two steps:

Step 1:

The menu contains the order “set 1. Point! ” (1)

Adjustment of the flow rate, with reference value of the wanted rate, usually flow rate =0 and entry of the number in the appointed unit. (2)

If the shown value of phase difference (3) does not change anymore, press “next” button. (4)

Step 2:

Adjustment of the flow rate, with the second reference value of the wanted second rate and entry of the number in the appointed unit.(5)


If the shown Value if phase difference does not change anymore, press “next” button.(4)

The calibration will be completed and the device will return automatically to the measured value display. If the calibration was correct, the measured value display will now show the second calibration value.

The calibration is now complete. With the button “exit” the calibration can be aborted any-time and the old calibration value will be kept. (6)

For fast calibration there is the option of zero balance.(7) By pressing the according button the present measurement value will be identified as zero value. The according offset will be added to the present calibration. The bracing of the characteristic line will be kept. After the zero point calibration the device will return automatically to the measured value display.

5.5. „Service“ – Measurement value control

EMD ps


φ_1 : <input style="width: 80%;" type="text" value="0.70"/> °	$\Delta\varphi_0$: <input style="width: 80%;" type="text" value="1.24"/> °
φ_2 : <input style="width: 80%;" type="text" value="-2.56"/> °	ϑ_0 : <input style="width: 80%;" type="text" value="25.84"/> °C
i : <input style="width: 80%;" type="text" value="96.84"/> mA	$\Delta\vartheta$: <input style="width: 80%;" type="text" value="-0.16"/> °C
U_1 : <input style="width: 80%;" type="text" value="0.06"/> V	$\Delta\varphi$: <input style="width: 80%;" type="text" value="3.26"/> °
U_2 : <input style="width: 80%;" type="text" value="0.06"/> V	v : <input style="width: 80%;" type="text" value="1.07"/> m/s

measure
system setup
channel setup
calibration
service


Single measurement values can be monitored under this sub menu. Furthermore additional information corresponding to the values of calibration and the present values are displayed. In the following these values are defined:

- φ_1 – phase-shift signal receiving coil 1
- φ_2 – phase-shift signal receiving coil 2
- i – induction current
- U_1 – voltage signal receiving coil 1
- U_2 – voltage signal receiving coil 2
- $\Delta\varphi_0$ – deviation of phase-shift difference in reference to the calibration
- ϑ_0 – core temperature in the moment of calibration
- $\Delta\vartheta_0$ – deviation of core temperature in reference to the calibration
- $\Delta\varphi$ – phase-shift difference between φ_1 and φ_2 (rough value)
- v – velocity of flow


6. Analog Output of EMD *ps*

The device has a passive analog 4-20 mA interface to evaluate the measurement signal. This interface can be energized externally by a supply voltage between 13,5V up to 26V DC. Preferably a customary in trade repeater with power supply should be foreseen.

Alternative 1:

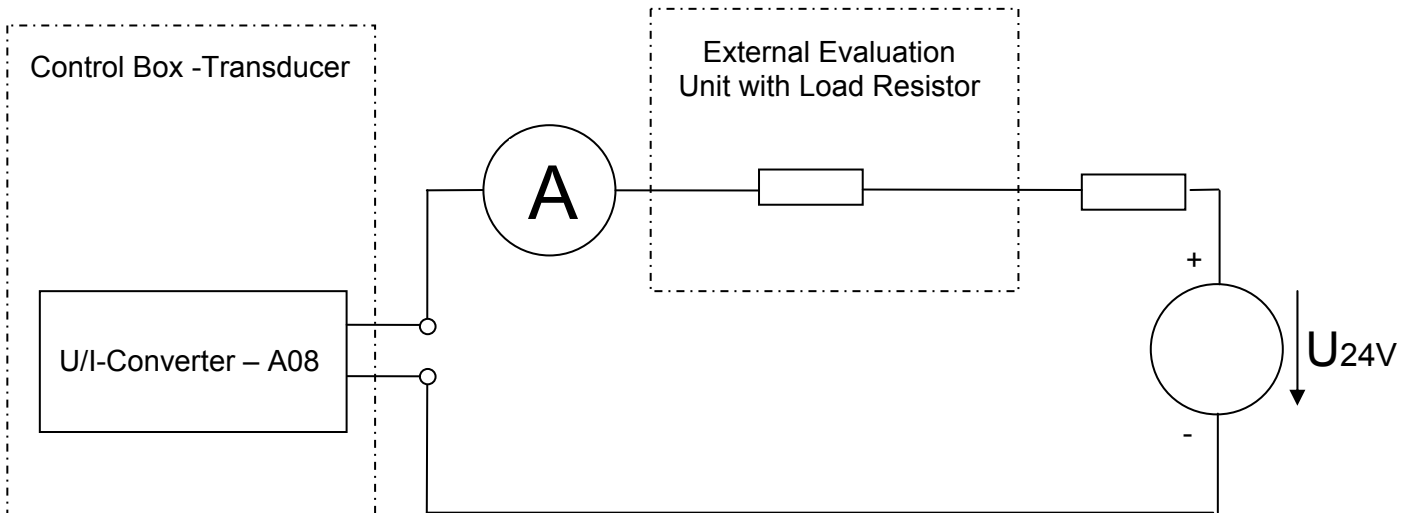

Alternative 2:

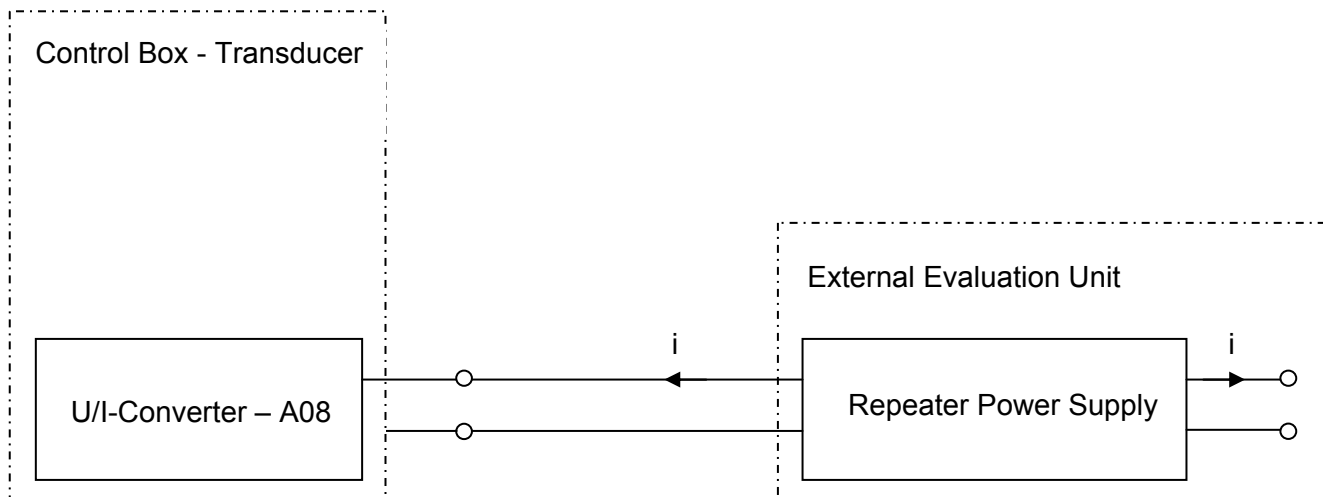

7. USB-Interface for Data Storage

For data storage you can connect an USB device at the USB port of the touch panel pc. The measurement date of the last two measurement days will be stored. Please wait for a minimum of 10 seconds before you unplug the USB device. Now the data location is in the folder "EMD-Data". The measurement data are saved as CSV-file and you can read them with the right application (like Excel). The structure of the data is built as follows:

timestamp	φ 1[°]	φ 2[°]	U1[V]	U2[V]
timestamp	φ 1[°]	φ 2[°]	current raw value	temperature raw value
timestamp	φ 1[°]	φ 2[°]	U1[V]	U2[V]
timestamp	φ 1[°]	φ 2[°]	current raw value	temperature raw value

for example

08:55:17.890	-6.639	-6.377	0.089	0.092
08:55:18.515	-6.634	-6.372	3.990	0.492
08:55:19.140	-6.631	-6.369	0.089	0.092
08:55:19.765	-6.631	-6.367	3.991	0.488

In order to built the real excitation current and the temperature you have to transform the raw values in the right way. You get the excitation current with:

$$\text{excitation current} = \text{current raw value} * 100.$$

With the following equation you can built the temperature.

$$\text{temperature} = \text{temperature raw value} * 40$$

8. Technical data sheet

Power Supply:

Supply Voltage:	230V AC
Power Input:	1 A (Switch on Current: 4 A)

Dimensions/Weight:

Dimension Transducer Control Box WxHxD:	400x800x300 Wall Fastening Box
Dimension Sensor Unit WxHxD:	215x20x510
Weight Transducer	35 kg
Weight Sensor	8,5 kg
Installation Standard Pipe	d _o 73 mm
Maximum of Cable Length between Sensor Unit and Transducer Box	20 m, More on Enquiry
Mounting Position Sensor Unit	In Any Order
Degree of Protection of Enclosure Sensor / Transducer:	IP54 / IP54

Fluid, external conditions:

Maximum Temperature Work Environment	0°C to 30°C
Maximum Relative Humidity Work Environment	<85%
Other Mounting Conditions	Indoor
Maximum Operating Temperature of Sensor	<500°C Fluid Temperature
Fluid	Liquid Metal Elec. Conductivity >10 ⁵ S/m and <=10 ⁷ S/m

Ranges:

Flow Range:	0,05 l/s – 10 l/s, Free of Blow Holes
Measures:	l/s, l/min, m ³ /h, kg/s, t/h (Other on Enquiry)
Pipe Dimensions:	Standard: 20 mm – 73 mm (Major Dimensions on Enquiry)
Excitation Frequency:	150 Hz – 800 Hz to Parameterize
Induction Current:	0 mA – 500 mA to Parameterize
Output Signal / Interfaces	4 – 20 mA
Measurement Uncertainty:	3% of Meas. Range under Condition of Constant and Balanced Temperature
Inlet Path:	5 x d _i (Inside Diameter)
Outlet Path:	3 x d _i (Inside Diameter)

Operation:

Display:	Touch Panel
Menu Item „Measure“:	Display of Measurement Value with Unit, Error Code, Recent Temperature of Sensor Core
Menu Item „System Setup“:	Input of System Parameters
Menu Item „Channel Setup“:	Input of Channel Parameters
Menu Item „Calibration“:	Two Point Calibration, Alternative: Zero Point Calibration
Menu Item „Service“:	Display of Additional Parameters

SAAS GmbH


Poistentalstraße 3
 01728 Bannewitz/ OT Possendorf
 Tel.: 035206/23871

name of construction: EMDps measuring transducer and sensor unit


manufacturer (firm): SAAS GmbH
 name of project: EMDps 73
 type: EMD-ps-MU500 & EMD-ps-S73
 responsible person of project: Marcel Flöter

create at: 12.04.2012
 edit at: 26.06.2012 by (abbreviation): saas_user

			Date	26.06.2012		SAAS GmbH	Cover page	= EMD + S1	Blatt: 1 / 10
			Ed.	saas_user		Poistentalstraße 3			
			Appr		EMDps measuring transducer and sensor unit	D-01728 Bannewitz / Germany		GB_tpI001	Seite:
Modification	Date	Name	Original		Replacement of	Replaced by			

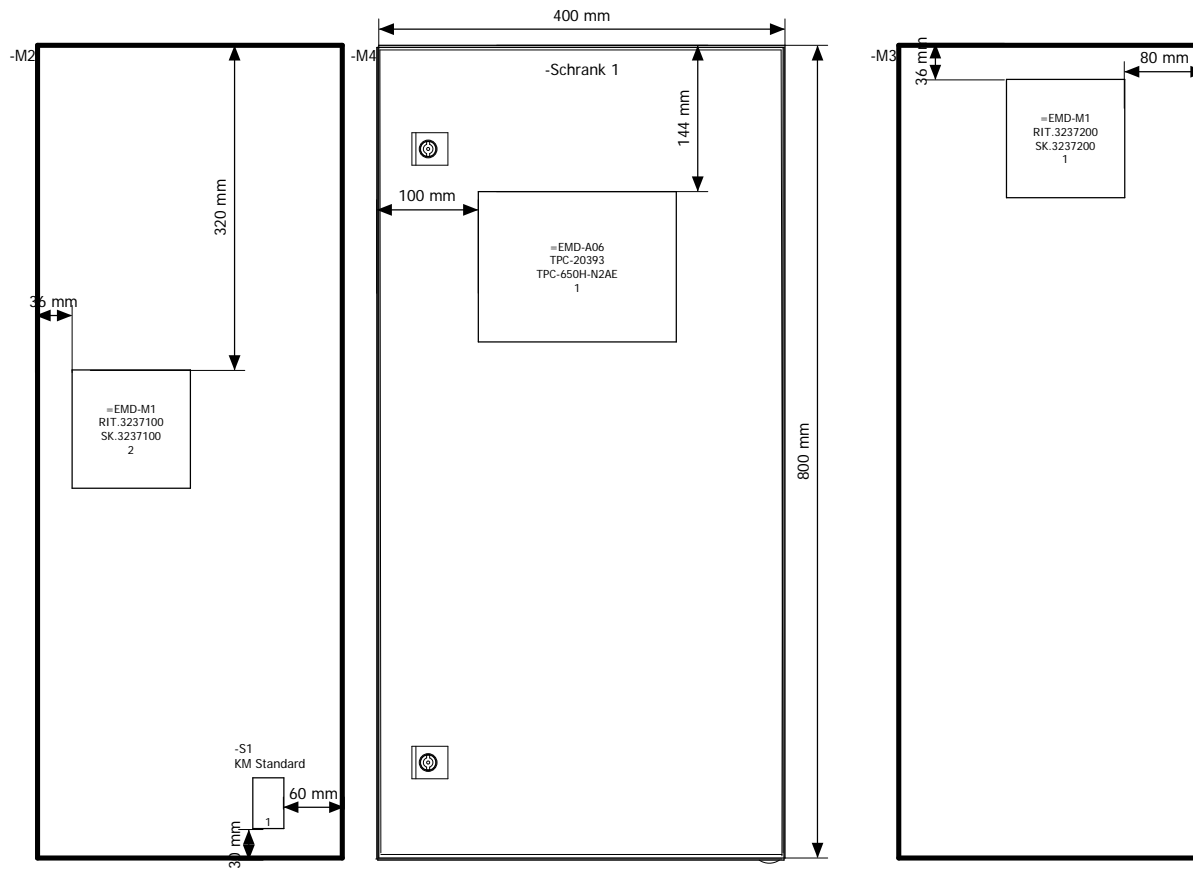

		Date	26.06.2012			SAAS GmbH	Control box overview	= EMD	
		Ed.	saas_user			Poisentalstraße 3		+ S1	
		Appr		EMDps measuring transducer and sensor unit		D-01728 Bannewitz / Germany		GB_tpI001	Blatt: 4 / 10
Date	Name	Original		Replacement of	Replaced by				Seite: 4

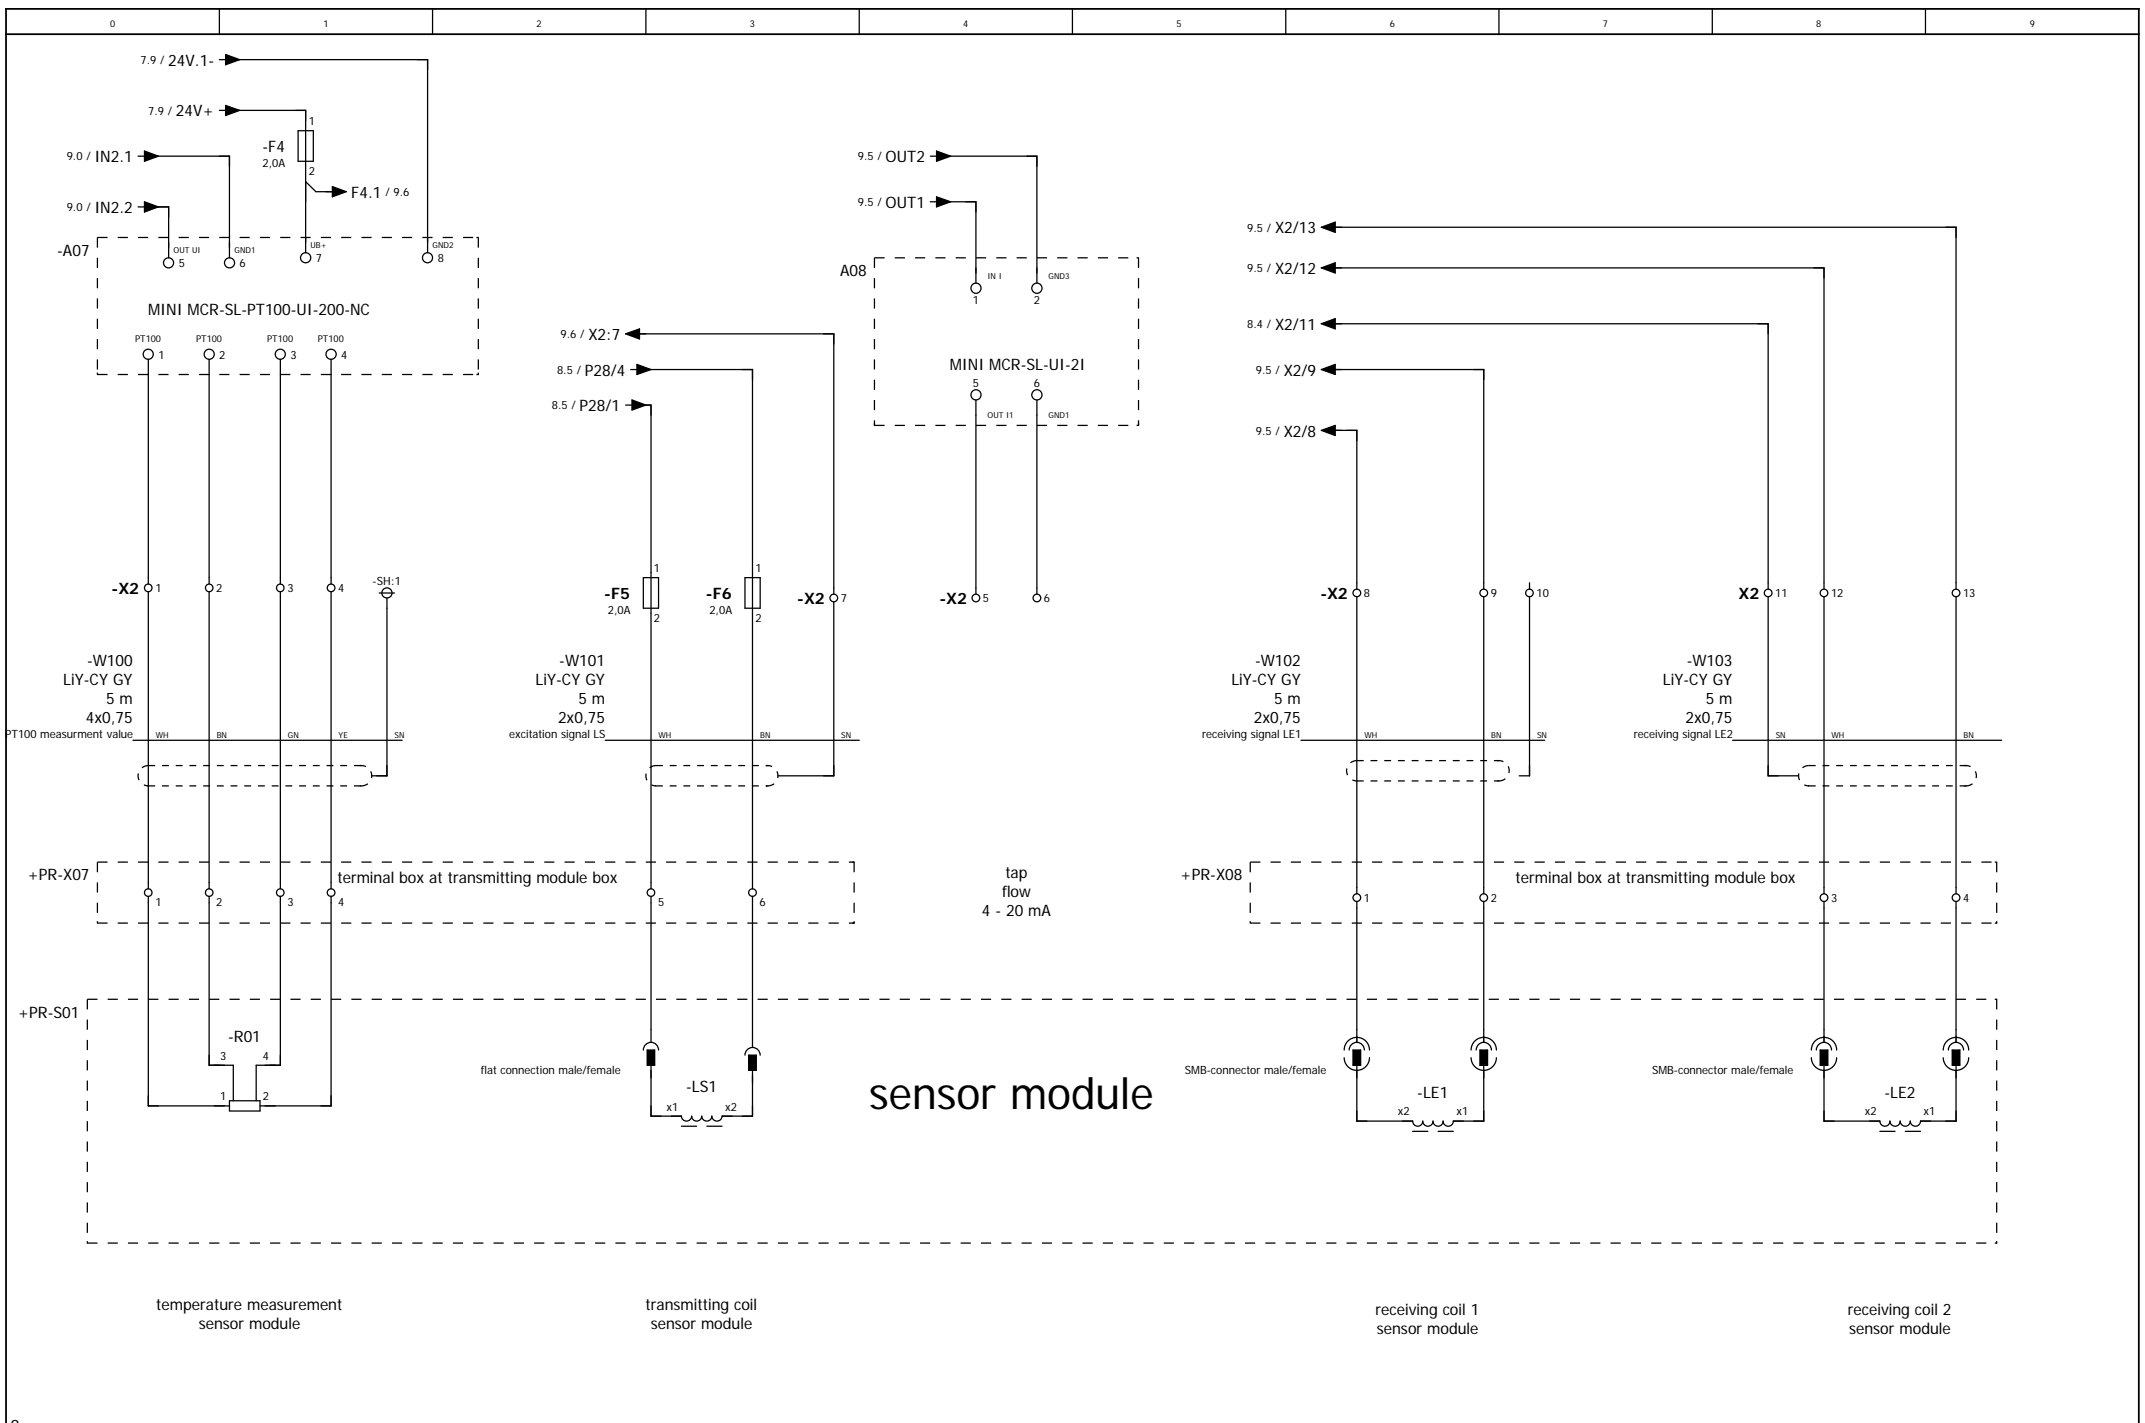

9		Date	26.06.2012	SAAS GmbH		Connection plan selector		= EMD
		Ed.	saas_user	Poientalstraße 3				+ S1
		Appr		D-01728 Bannewitz / Germany				Blatt: 10 / 10
Modification	Date	Name	Original	Replacement of	Replaced by	GB_tp001		Seite: 10

EMDps measuring transducer and sensor unit

Notes:

SAAS – Systemanalyse & Automatisierungsservice GmbH
Poientalstraße 3, D-01278 Bannewitz
Tel.: 035206 23871
Fax: 035206 23828
e-mail: info@saas-online.de
web: www.saas-online.de